

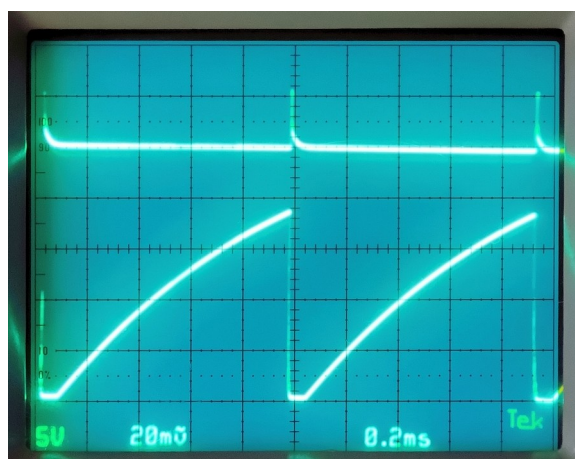
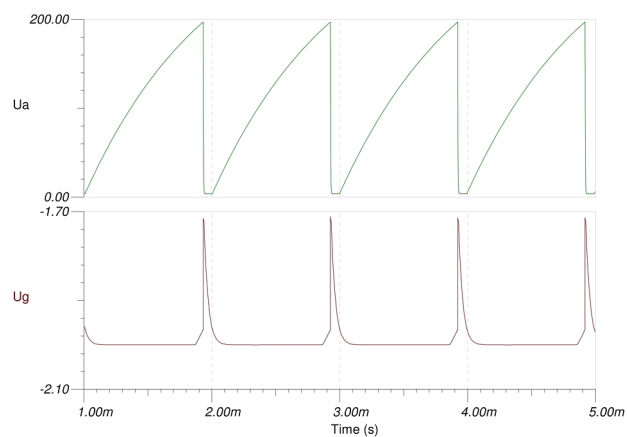
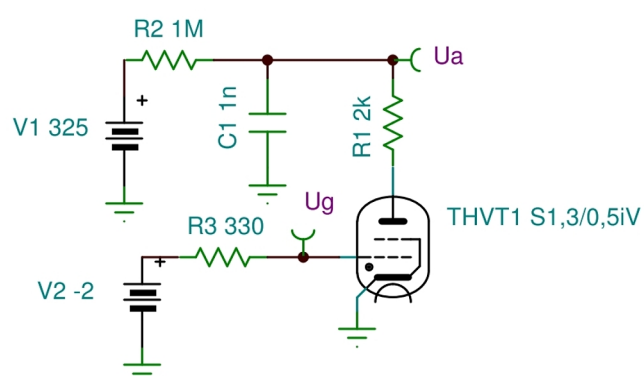


S1,3/0,5iV /WF GDR/ Thyatron Macro Model

Thyatron relaxation oscillator:

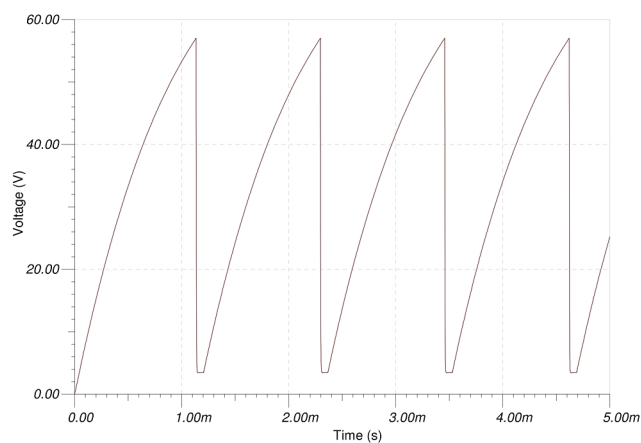

**This model is valid for the following thyatrons (within max. ratings):
PL21, 2D21, 21TE31**

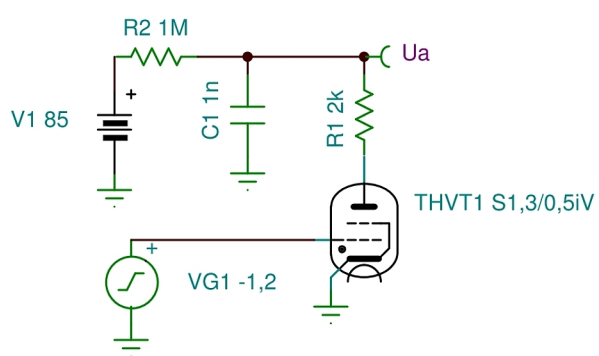

Timebase circuit of early oscilloscopes:

